

HPLC REPORT

Sample Description:

Structure : TH-33-NH₂
 Number : 0200046
 Lot # : LT151223-LT288450
 Column : 4.6mm*250mm, kromasil C18-5
 Mobile Phase : A=0.1% TFA/Acetonitrile,
 : B=0.1%TFA/water,


Gradient :

	A	B
0.01min	23%	77%
25.0min	48%	52%
25.1min	100%	0%
30.0min	STOP	

Flow rate : 1.0ml/min


Wavelength : 220nm

Volume : 10ul

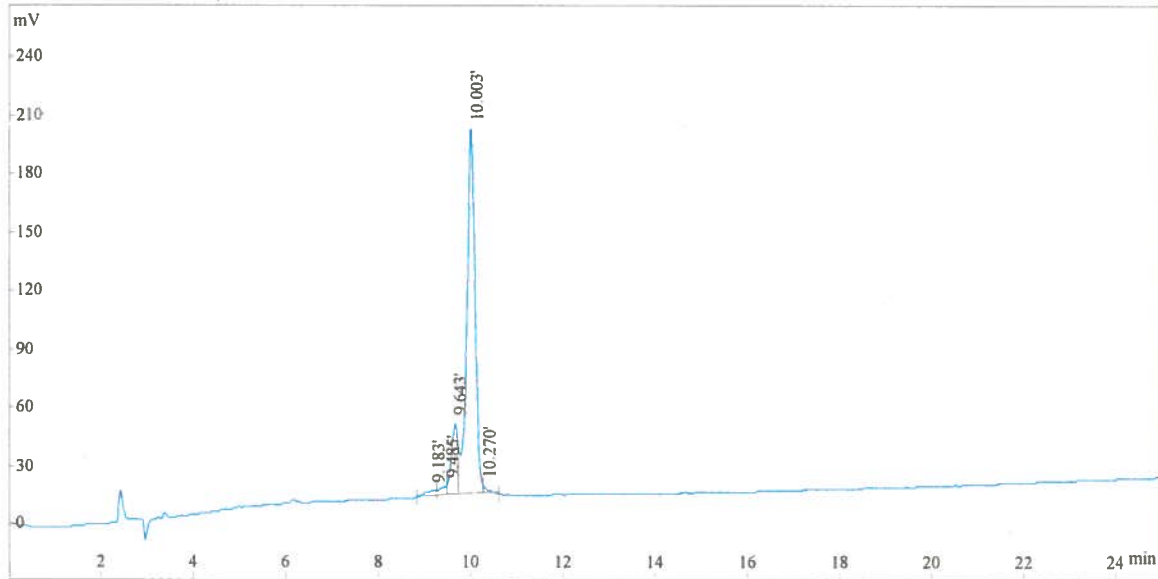

Rank	Time	Conc.	Area	Height
1	9.183	1.8219	52120	3266
2	9.485	1.9681	56302	5865
3	9.643	12.7313	364203	37426
4	10.003	82.4184	2357738	189860
5	10.270	1.0603	30332	4169
Total		100	2860695	240586

Mass Spectrometry Report

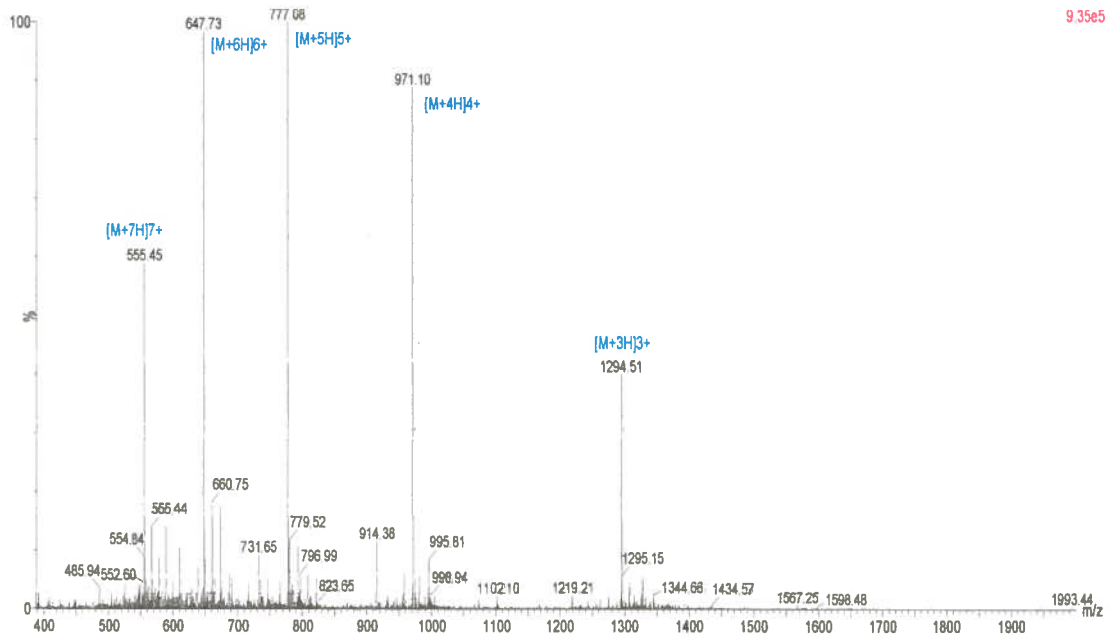

9.35e5

Sample: 288450

MW: 3878.54

Item	Parameter	Item	Parameter
Probe:	ESI	Probe bias:	+4.5kv
Nebulizer Gas Flow:	1.5L/min	Detector:	1.5kv
CDL:	-20.0v	T.Flow:	0.2ml/min
CDL Temp:	250°C	B.conc:	50%H2O50%ACN
Block Temp:	200°C		